DAVID SCOTT COMPANY

PATIENT TRANSFER DEVICE IFU

Instructions for Use

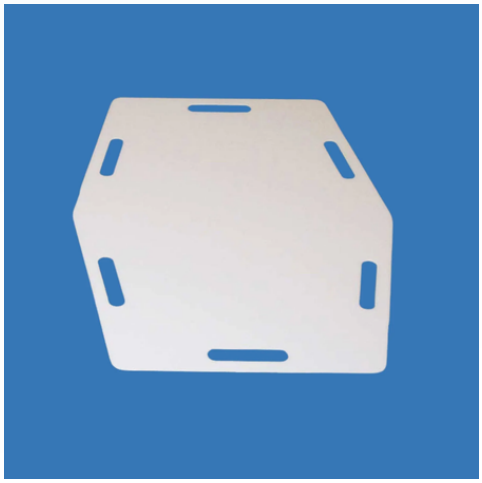

REF **4755XL**

INTENDED USE: Intended use if for personnel to effortlessly slide patient from one gurney or table to another, eliminating risk of back injury while increasing patient comfort dramatically. The intended users of this device are medical professionals within hospitals and surgery centers.

GENERAL INFORMATION

- Product not made with Natural Rubber Latex
- Product warranty covers product from manufacturing defects for period of 2 years
- If damaged in shipping, call Customer Service at (508) 875-3333 to obtain Return Material Authorization number. For product warranty issues, contact Customer Service.
- Life of device is 5 years under normal use
- Store device between -4°F to +86°F (-20°C to 30°C)

COMPONENT OVERVIEW

Patient Slide enables personnel to easily slide patient from one bed to another.

INSTRUCTIONS

Become familiar with the features of patient positioning device before use with a patient. Always practice use on a nurse, physician or appropriate volunteer prior to using clinically.

Clean Sheet Transfer

1. Lock stretcher against procedure table, gently pull draw sheet up, tilting patient up on side. Position Slide under draw sheet, then lower patient down
2. Using draw sheet, steadily slide patient over Slide to transfer table
3. Gently remove Slide from beneath patient

Soiled Sheets Transfer

1. Lock stretcher against procedure table, take a clean draw sheet and wrap it around Slide covering three quarters of slide bottom
2. Gently tilt patient up on side, leaving soiled sheets down. Position Slide and clean draw sheet beneath patient, directly under torso
3. Medic #1 pulls draw sheet, white Medic #2 pushes patient, sliding patient over Slide onto transfer table
4. Remove Slide from beneath patient

DAVID SCOTT COMPANY PATIENT TRANSFER DEVICE- PATIENT SHIFTER

Cleaning Instruction

Spray and wipe clean with hospital approved disinfectant

GENERAL SPECIFICATIONS

Device Dimensions (maximum)

- Length: 33” +/- 0.5” (84 cm +/- 1 cm)
- Width: 22” +/- 0.5” (56 cm +/- 1 cm)
- Depth: 1/16” +/- 0.5” (.16 cm +/- 1 cm)
- Device Weight: 1 +/- 0.5 lbs. (.45 +/- .22 kg)

DISPOSAL

- General - Prevent infection by cleaning and disinfecting product before disposal
- Packaging - Dispose packaging material via household waste according to national requirements

PRODUCT USE WARNINGS

WARNING! Hazard resulting from incorrect use.

WARNING! Do not reuse device if there are obvious signs of damage or functional issues. Consult manufacturer before reusing.

USER NOTICE Any serious incident that has occurred in relation to the device should be reported to the manufacturer and the competent authority of the Member State in which the user and/or patient is established.